

FIG. 1A

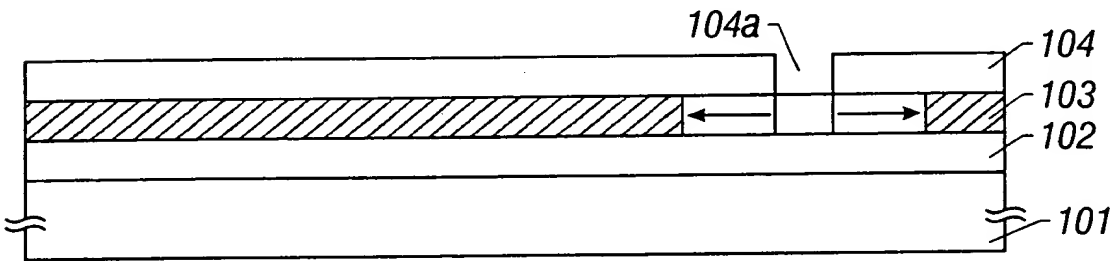


FIG. 1B

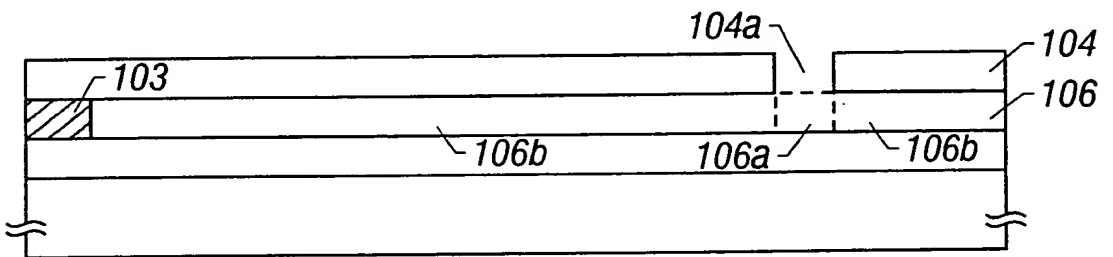


FIG. 1C

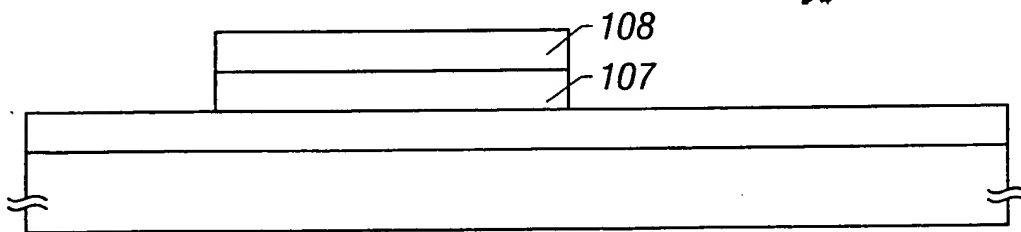


FIG. 1D

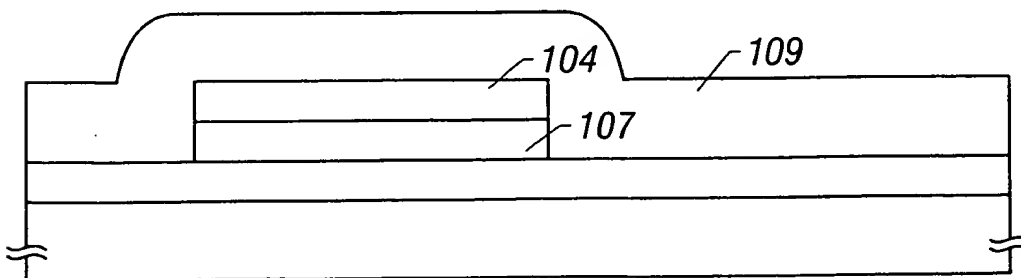


FIG. 1E

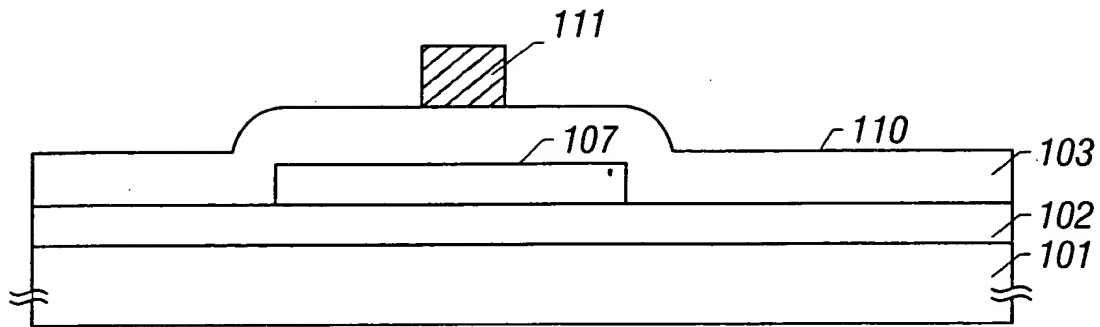


FIG. 2A

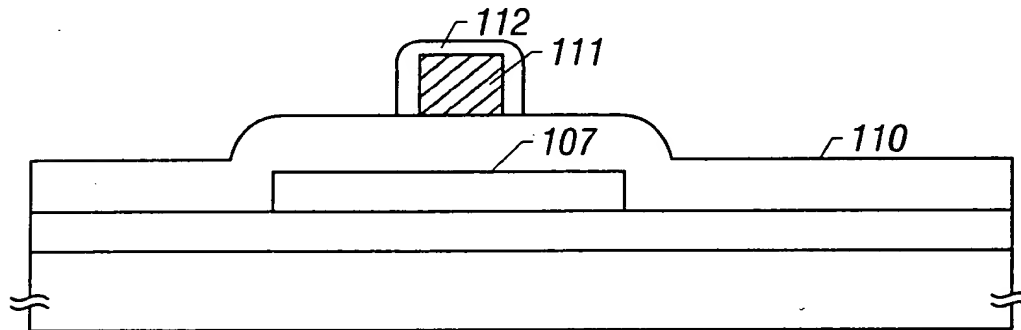


FIG. 2B

DOPANT ION IMPLANT

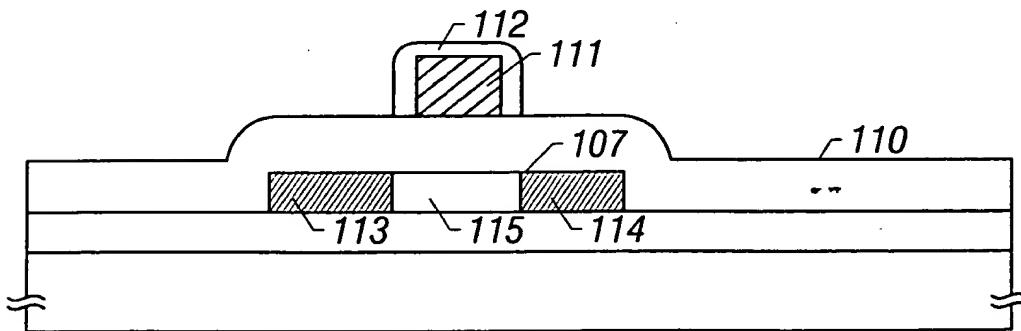


FIG. 2C

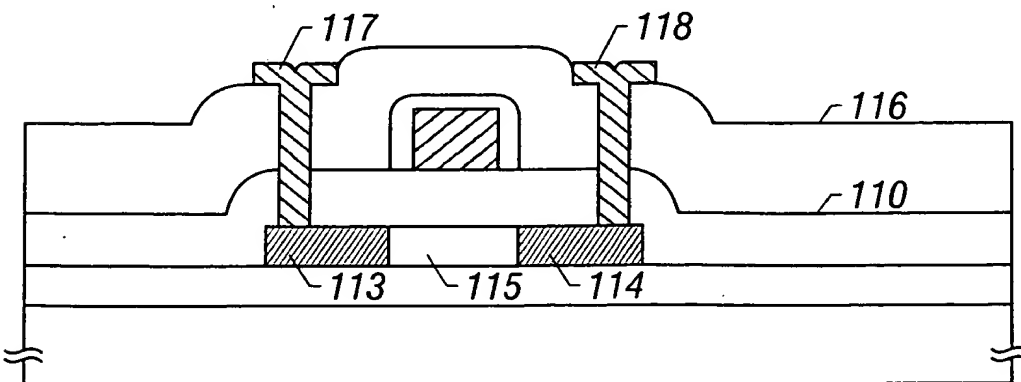


FIG. 2D

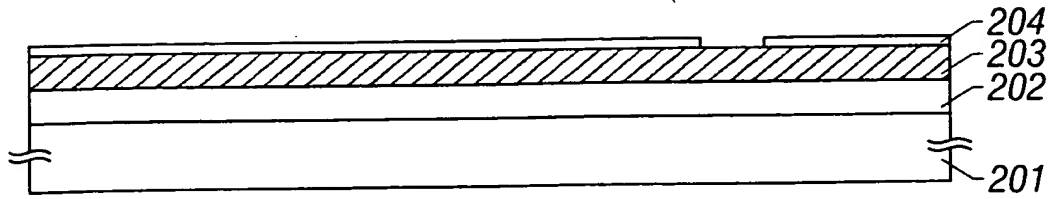


FIG. 3A

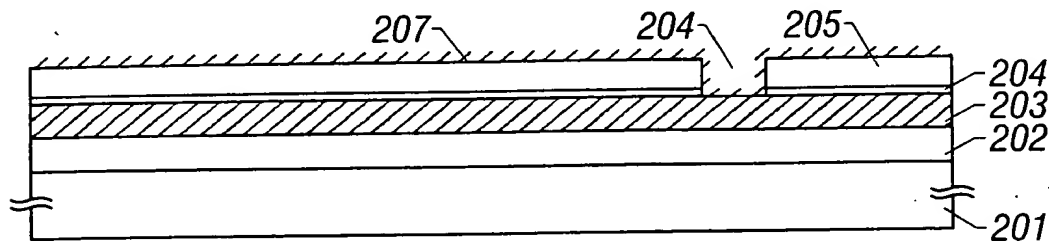


FIG. 3B

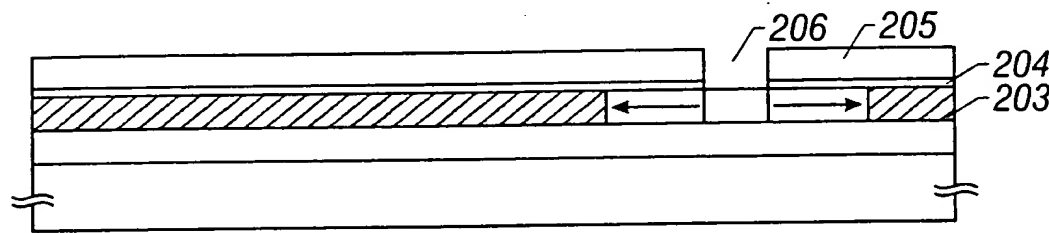


FIG. 3C

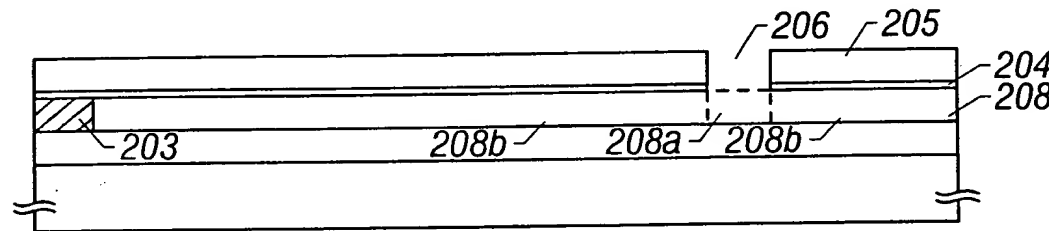


FIG. 3D

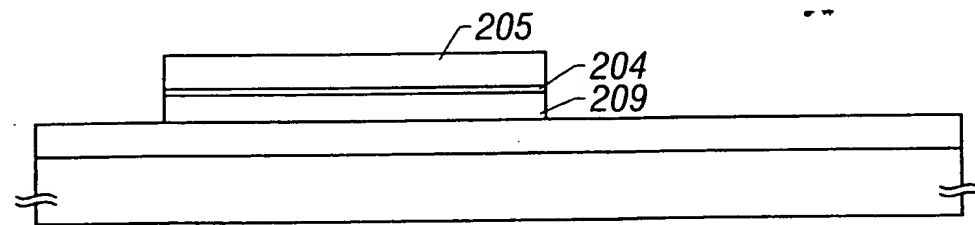


FIG. 3E

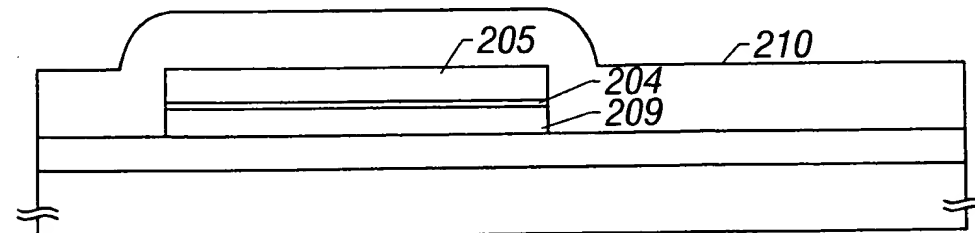


FIG. 3F

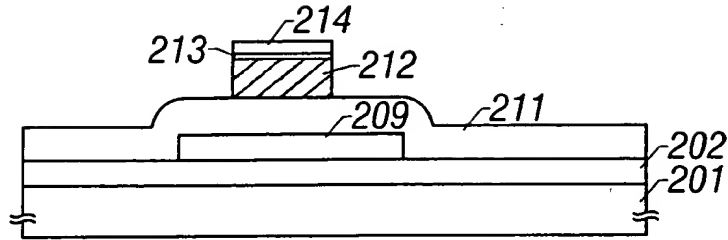


FIG. 4A

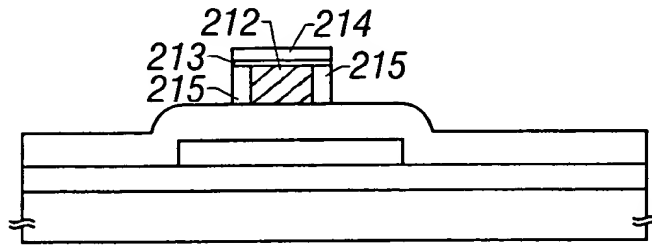


FIG. 4B

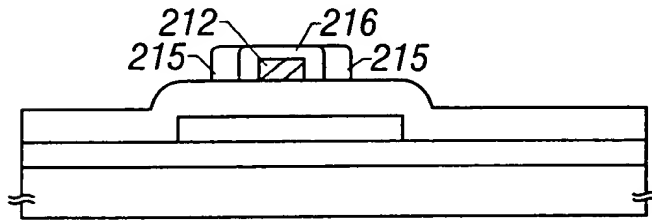


FIG. 4C

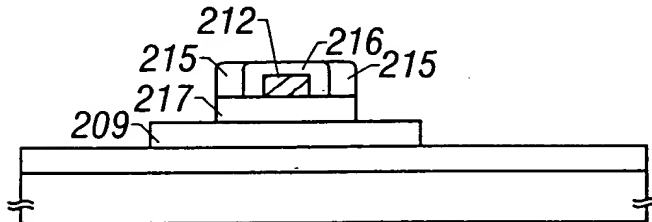


FIG. 4D

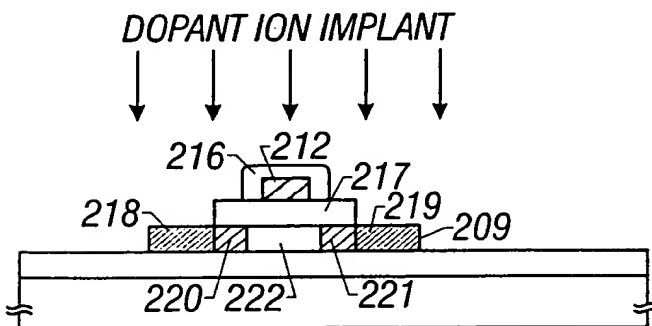


FIG. 4E

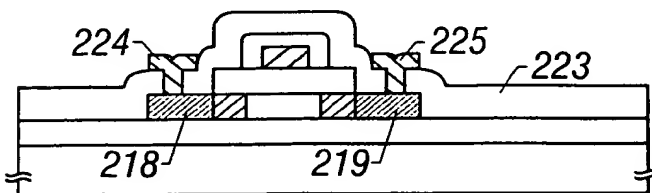


FIG. 4F



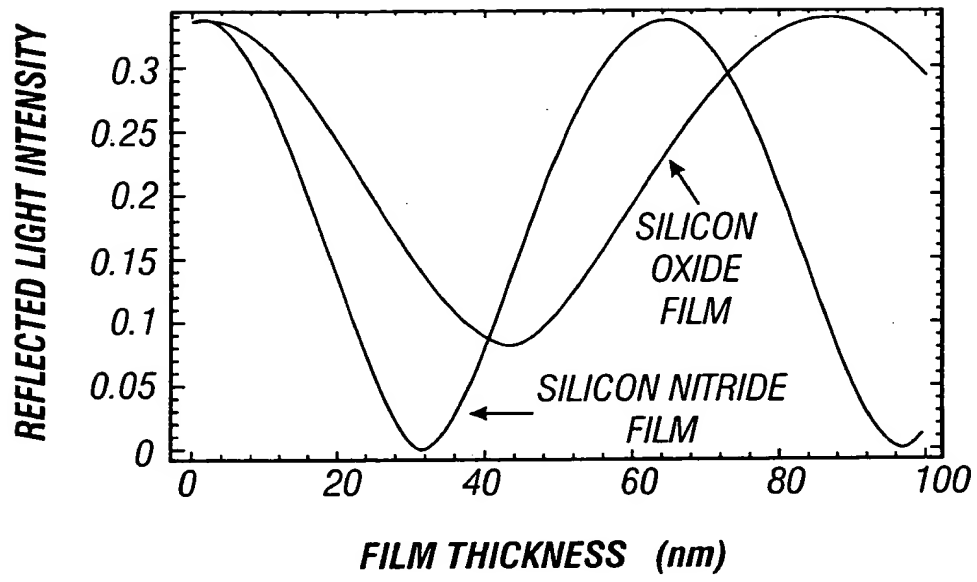



FIG. 5

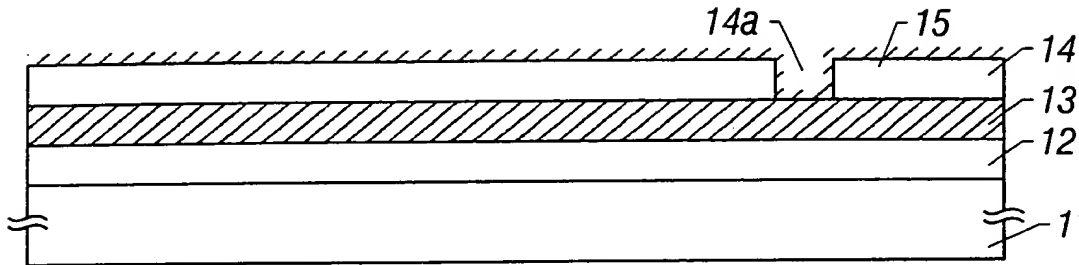


**FIG. 6A**  
**(Prior Art)**

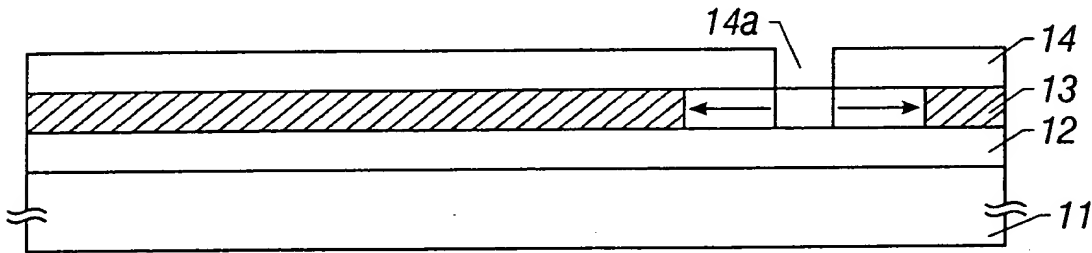

**FIG. 6B**  
**(Prior Art)**

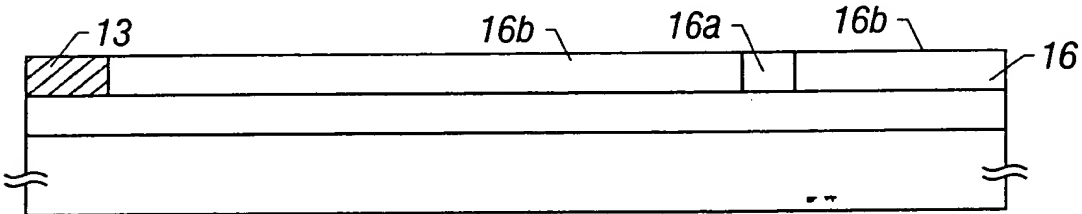

**FIG. 6C**  
**(Prior Art)**

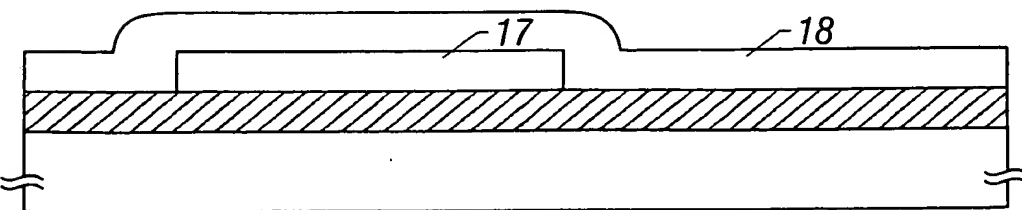

**FIG. 6D**  
**(Prior Art)**